



3M™ Curoso™ Disinfecting Port Protectors

Achieved a 99.99% reduction in 6 microbes commonly associated with CLABSI

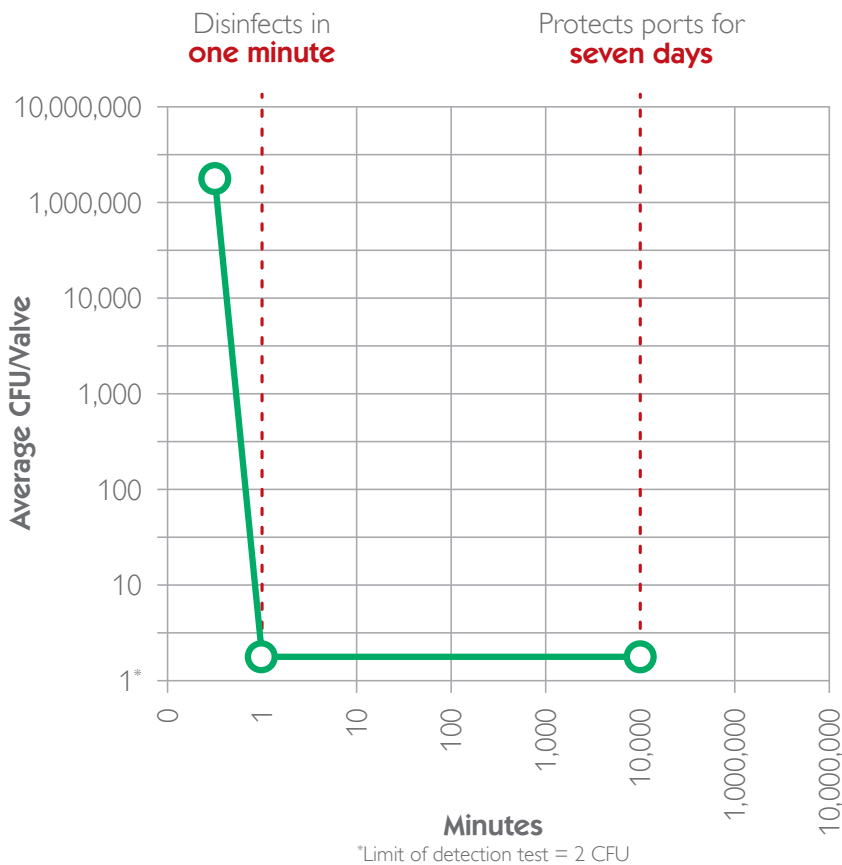

The effectiveness of Curoso products was tested in vitro against^{1,2}:




Staphylococcus aureus



Staphylococcus epidermidis



Escherichia coli



Candida albicans



Pseudomonas aeruginosa



Candida glabrata

Study conclusion:

1. All test samples exceeded the minimum 4-log reduction after **one minute**.

Studies were conducted at independent laboratories. 3M data on file.

¹ For more information regarding organisms associated with catheter-related bloodstream infections, refer to Wenzel RP and Edmond MB. The Impact of Hospital-Acquired Bloodstream Infections. Emerg Infect Dis. 2001 Mar Apr;7(2):174-7.

² Data reflects in vitro findings on Curoso™ Disinfecting Port Protectors conducted by an independent laboratory.



Curoso™ is a trademark of 3M Company. Vygon (UK) Ltd accepts no liability for the content of this poster or for the consequences of any actions taken on the basis of the information provided.

3M
Authorised Distributor
Medical Products